


Summary Results for Mean Corpuscular Volume for All Participants

MEAN CORPUSCULAR VOLUME (MCV) IN ALL SUBJECTS

PARTICIPANTS=65877, MEAN=90.36, STANDARD DEVIATION=4.97


1st PERCENTILE=77.00, MEDIAN=91.00, 99th PERCENTILE=102.00

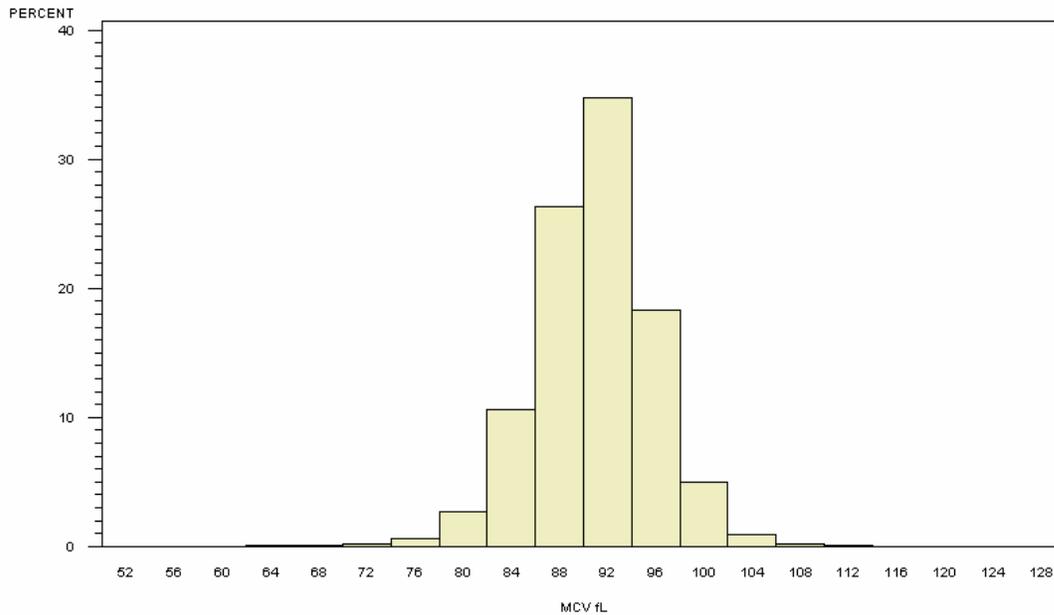

NORMAL RANGE 80-98 fL, TAKEN FROM Labcorp Sample Test

MEAN CORPUSCULAR VOLUME (MCV) IN ALL SUBJECTS

BY MCV CATEGORY WITHIN GENDER (PARTICIPANTS=65877)

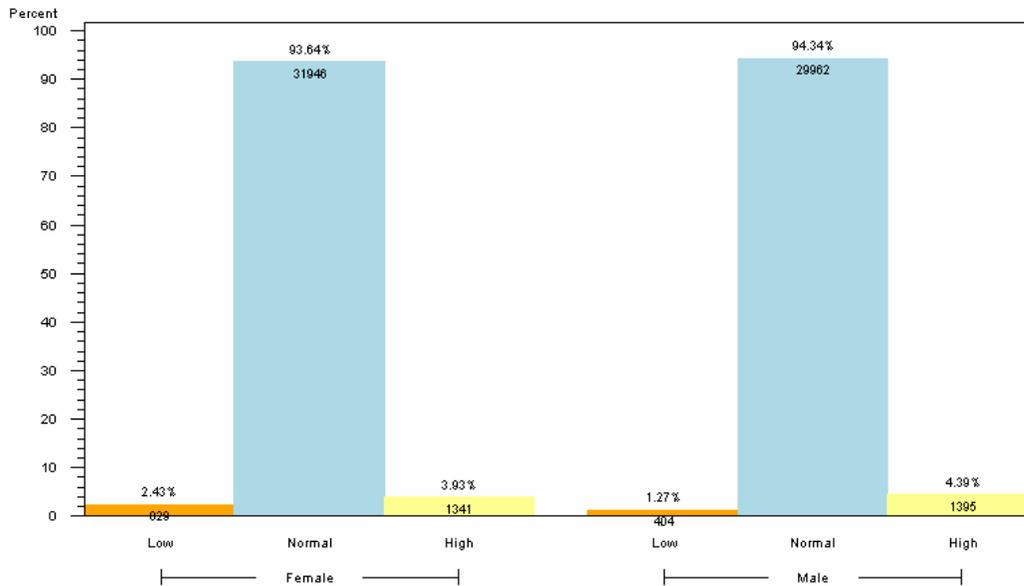

1. LOW <80, NORMAL 80-98, HIGH >98
2. RANGES TAKEN FROM Labcorp Sample Test
3. RESULTS BASED ON LAB VALUES, NOT DIAGNOSIS

Reader's Guide to Understanding This Information:

More than 90% of all participants had MCV levels within the expected range.