


Summary Results for Platelets for Participants of All Ages

PLATELET COUNT IN ALL SUBJECTS


PARTICIPANTS=65736, MEAN=283.81, STANDARD DEVIATION=69.97
 1st PERCENTILE=151.00, MEDIAN=276.00, 99th PERCENTILE=483.00

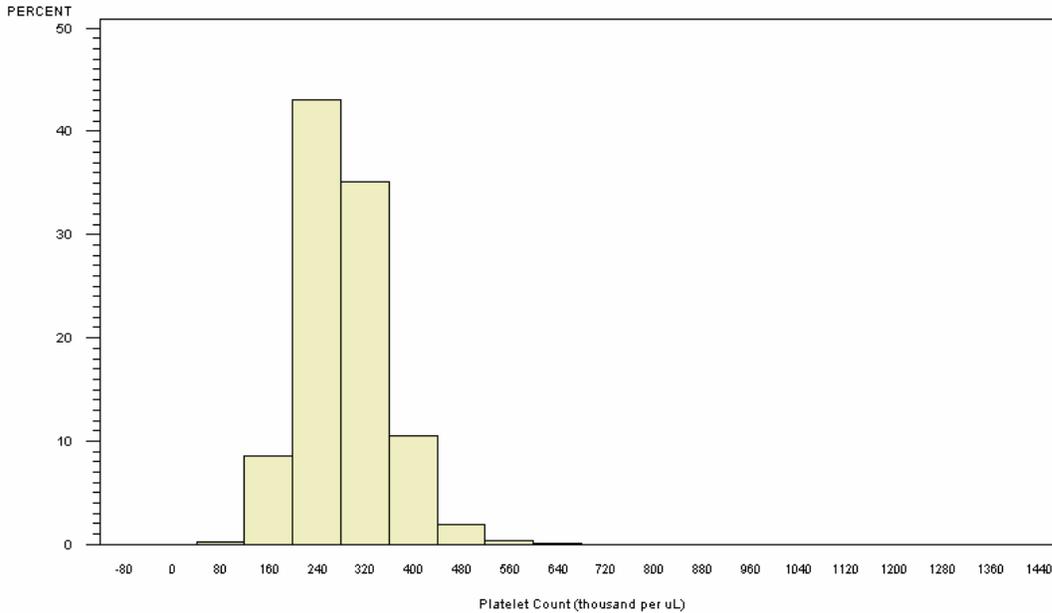

NORMAL RANGE 140-415 $10^3/\mu\text{L}$, TAKEN FROM Labcorp Sample Test

PLATELET COUNT IN ALL SUBJECTS

BY PLATELETS CATEGORY WITHIN GENDER (PARTICIPANTS=65736)

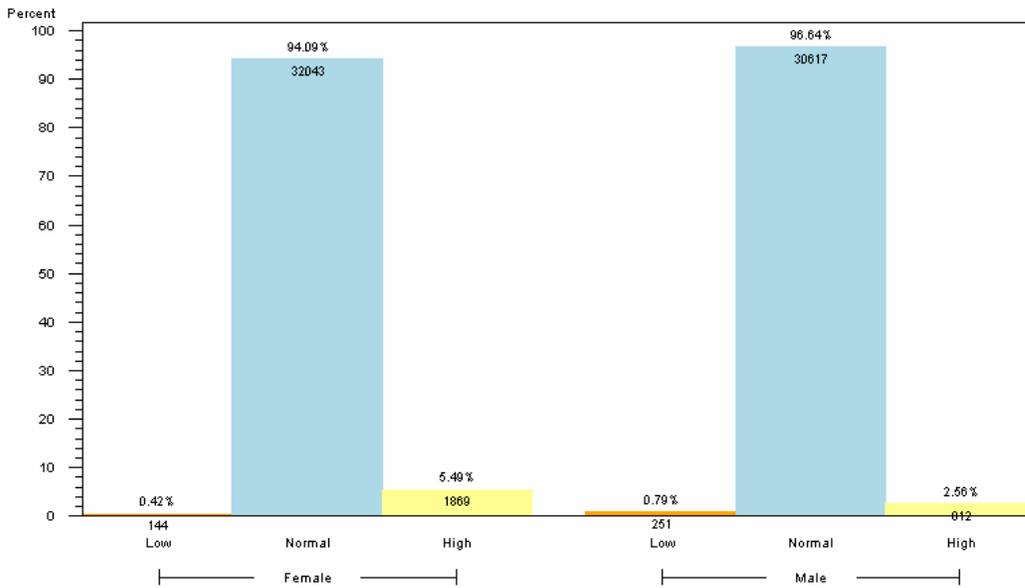

1. LOW <140, NORMAL 140-415, HIGH >415 (UNIT: $10^3/\mu\text{L}$)
2. RANGES TAKEN FROM Labcorp Sample Test
3. RESULTS BASED ON LAB VALUES, NOT DIAGNOSIS

Reader's Guide to Understanding This Information:

Approximately 95% of all participants had platelet levels within the expected range. A slightly higher proportion of females compared to males had elevated platelet levels.