


Summary Results for Mean Corpuscular Hemoglobin Concentration for All Participants

MEAN CORPUSCULAR HEMOGLOBIN CONCENTRATION (MCHC) IN ALL SUBJECTS


PARTICIPANTS=65877, MEAN=33.80, STANDARD DEVIATION=0.65
 1st PERCENTILE=32.10, MEDIAN=33.80, 99th PERCENTILE=35.30

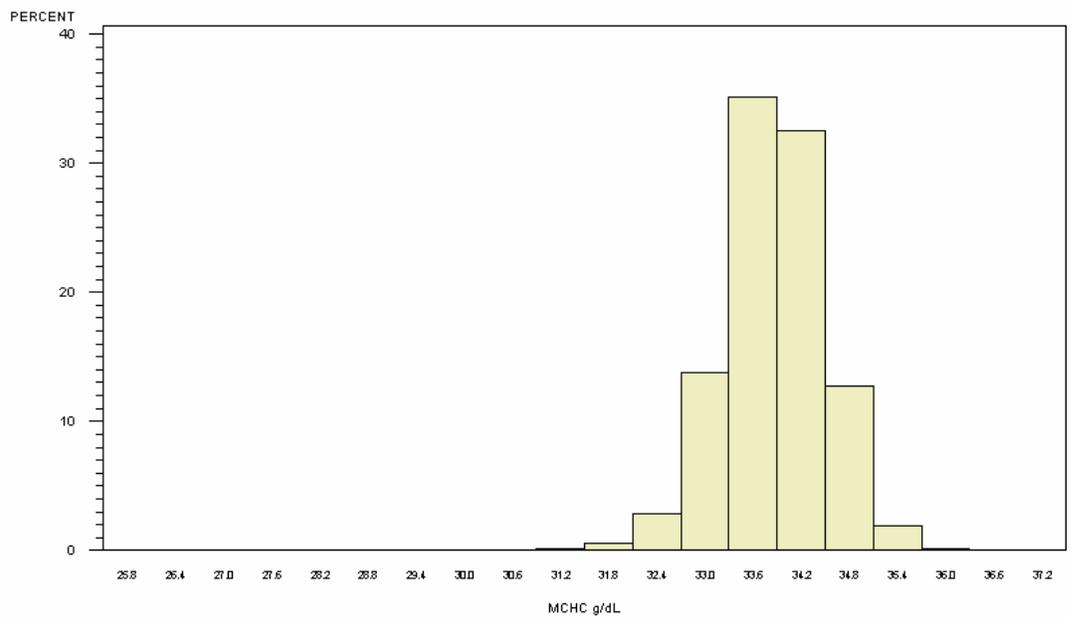

NORMAL RANGE 32-36 g/dL, TAKEN FROM Labcorp Sample Test

MEAN CORPUSCULAR HEMOGLOBIN CONCENTRATION (MCHC) IN ALL SUBJECTS

BY MCHC CATEGORY WITHIN GENDER (PARTICIPANTS=65877)

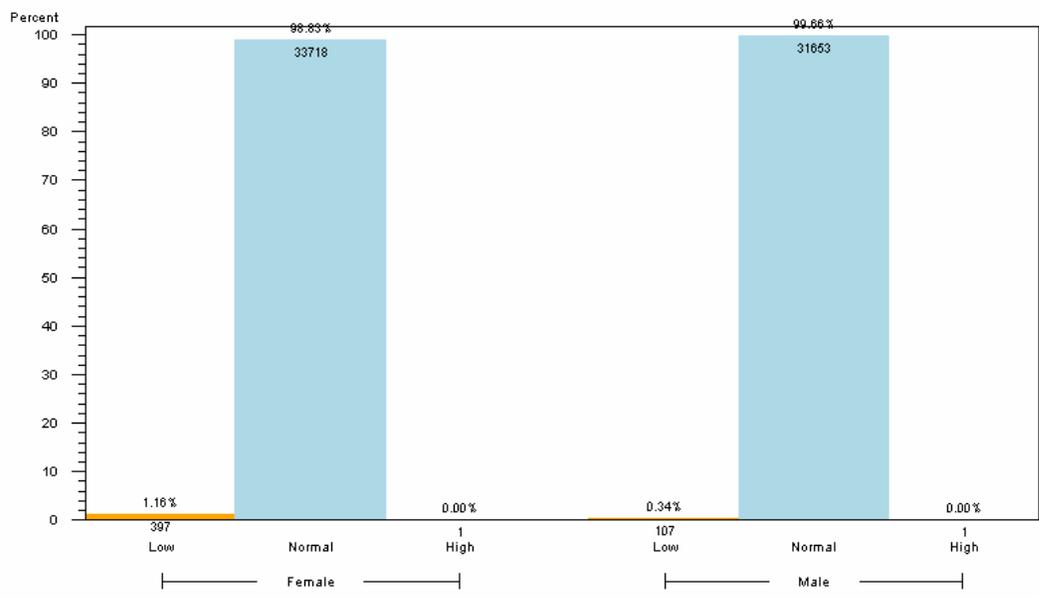

1. LOW <32, NORMAL 32-36, HIGH >36
2. RANGES TAKEN FROM Labcorp Sample Test
3. RESULTS BASED ON LAB VALUES, NOT DIAGNOSIS

Reader's Guide to Understanding This Information:

More than 95% of all participants had MCHC levels within the expected range.